


REPLACEMENT SHEET

1/16


FIG. 1

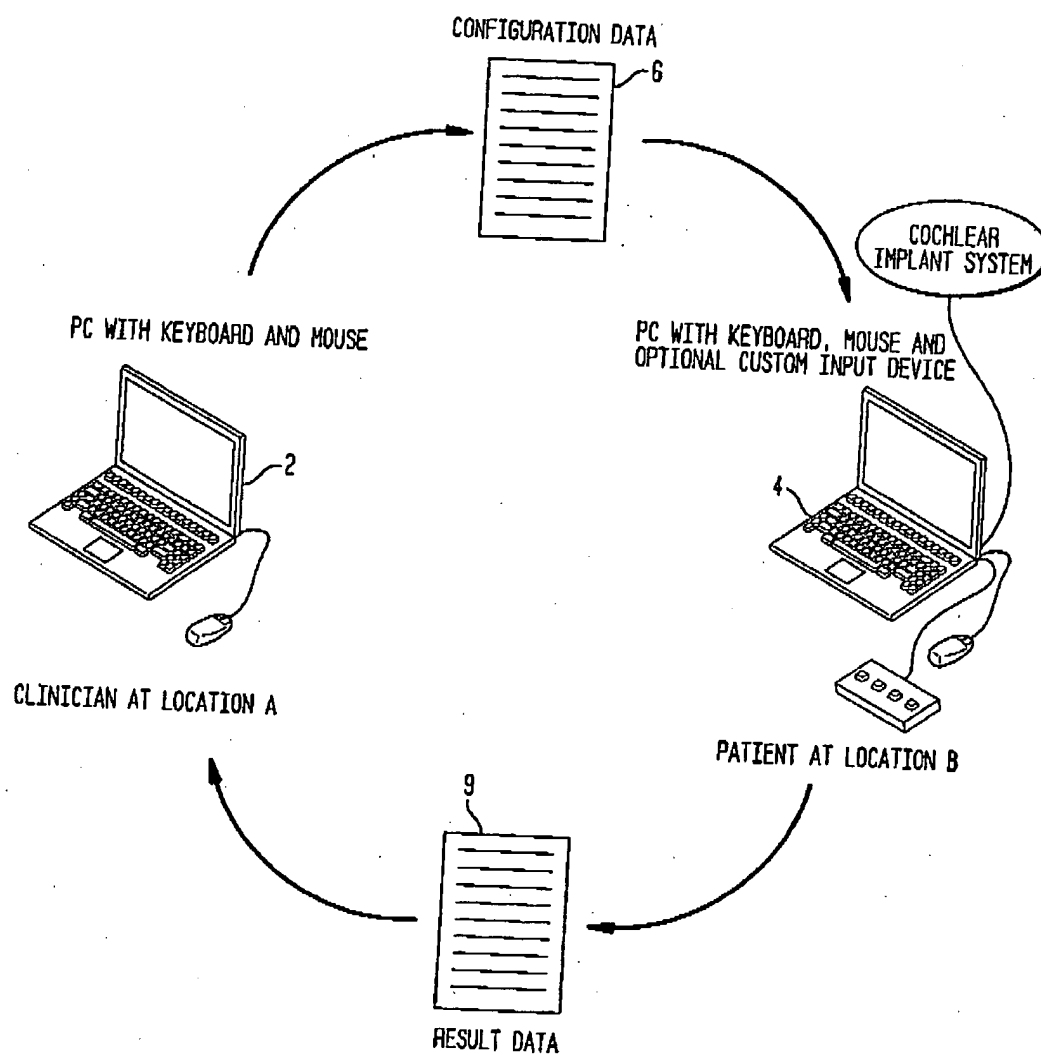

REPLACEMENT SHEET


2/16

FIG. 1A

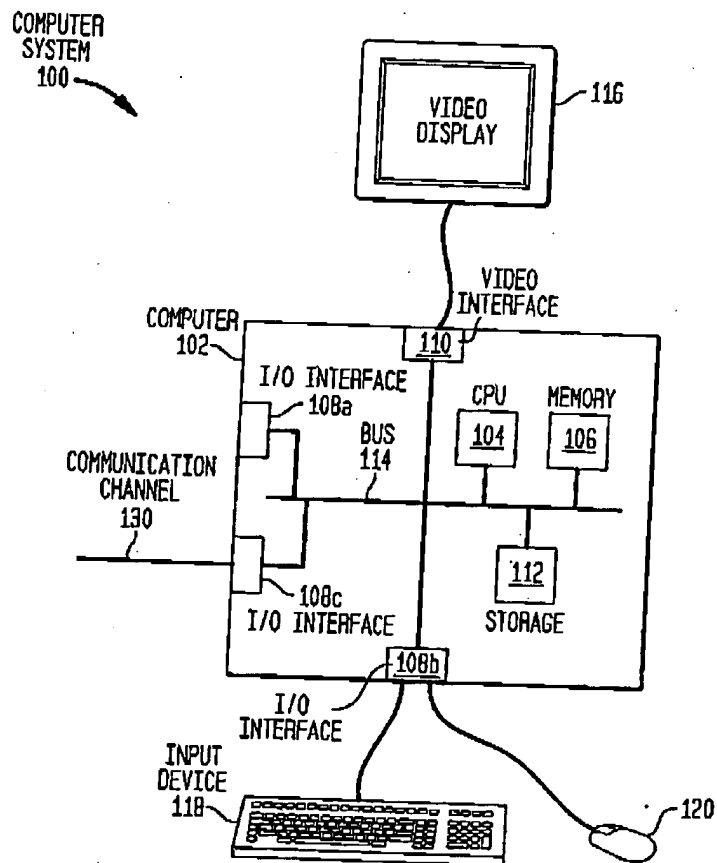

3/16


FIG. 2

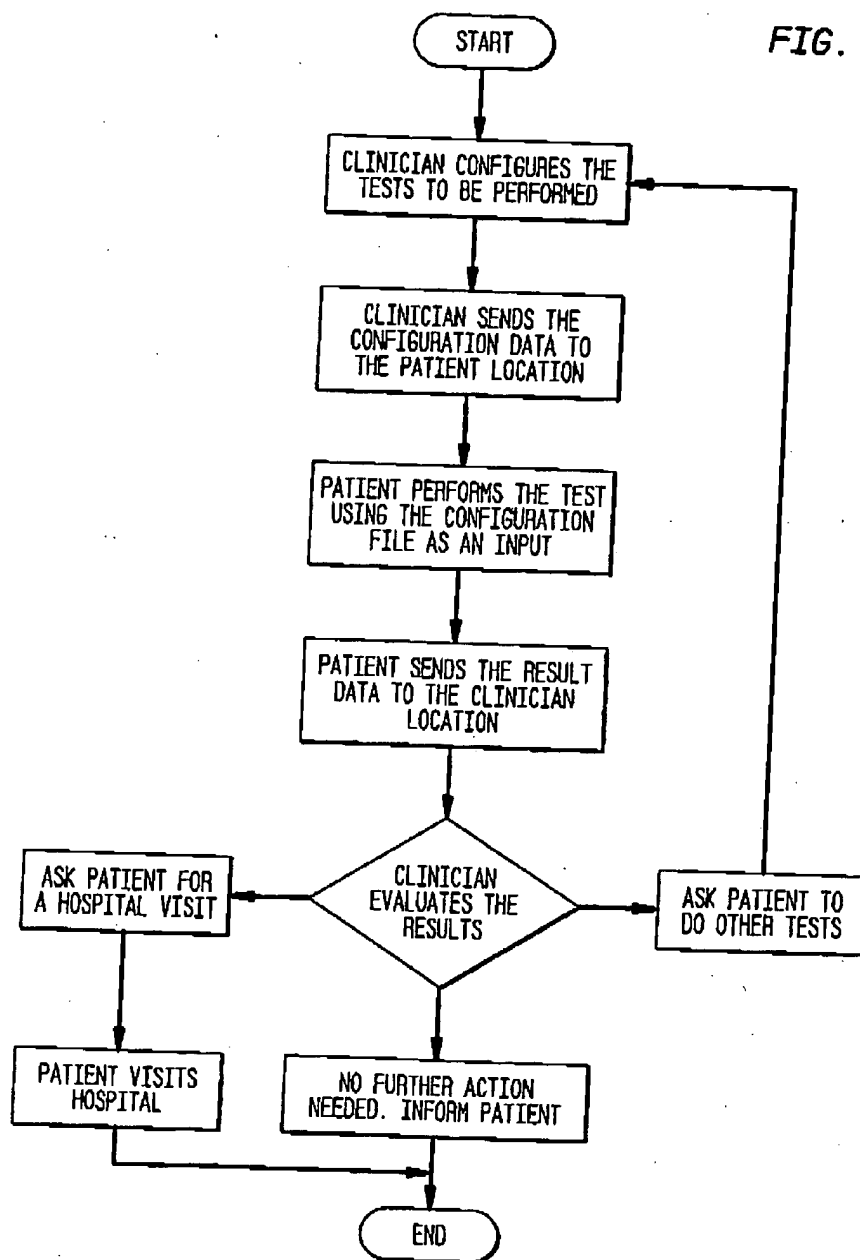

4/16

NEW SHEET

FIG. 3

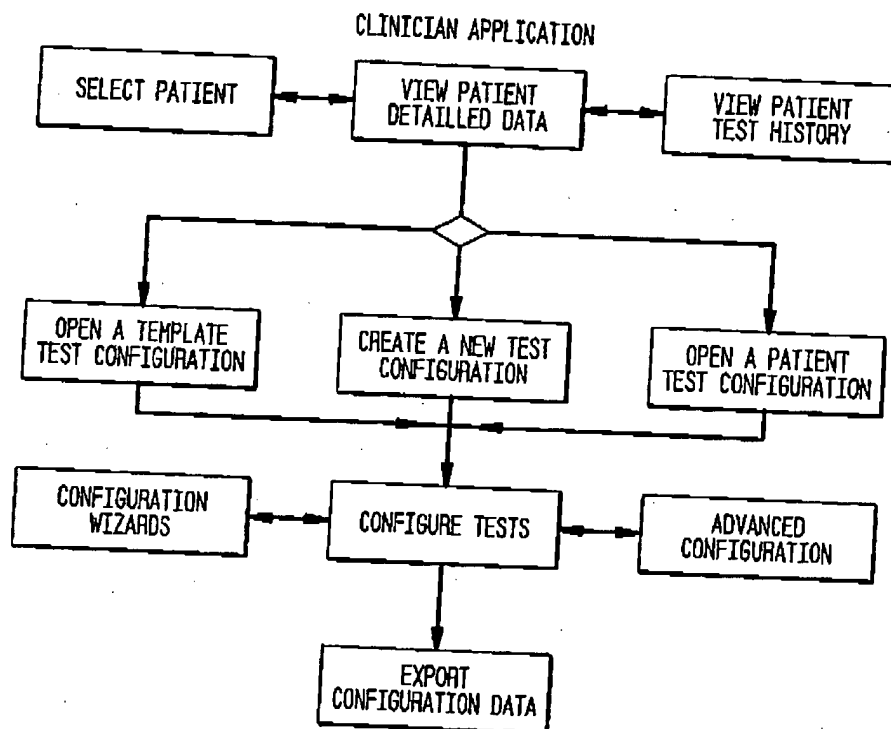

REPLACEMENT SHEET

5/16

FIG. 4

Automated Clinical Assistant Prototype v1.0

1) Recipient: Bob Peters

2) Language: English

3) SP connection: Test

4) Tests to be performed:

- ☒ System Integrity
- ☐ T-WRT
- ☒ T-levels
- ☐ C-levels
- ☐ Loudness balancing
- ☐ Pitch ranking
- ☐ Phoneme discrimination

5) Maps to be used:

slot1 slot2 slot3

Save this configuration for remote execution.

Save

Start the recipient's interface.

Go

FIG. 15

Automated Clinical Assistant Prototype v1.0

Test results for Bob Peters:

- ☒ System Integrity OK
- ☐ T-WRT
- ☒ T-levels NOT OK
- ☐ C-levels
- ☐ Loudness balancing
- ☐ Pitch ranking
- ☐ Phoneme discrimination

Detailed report:

View

Save

Print

Back tests:

Back


Close the application:

End

6/16


REPLACEMENT SHEET

FIG. 5

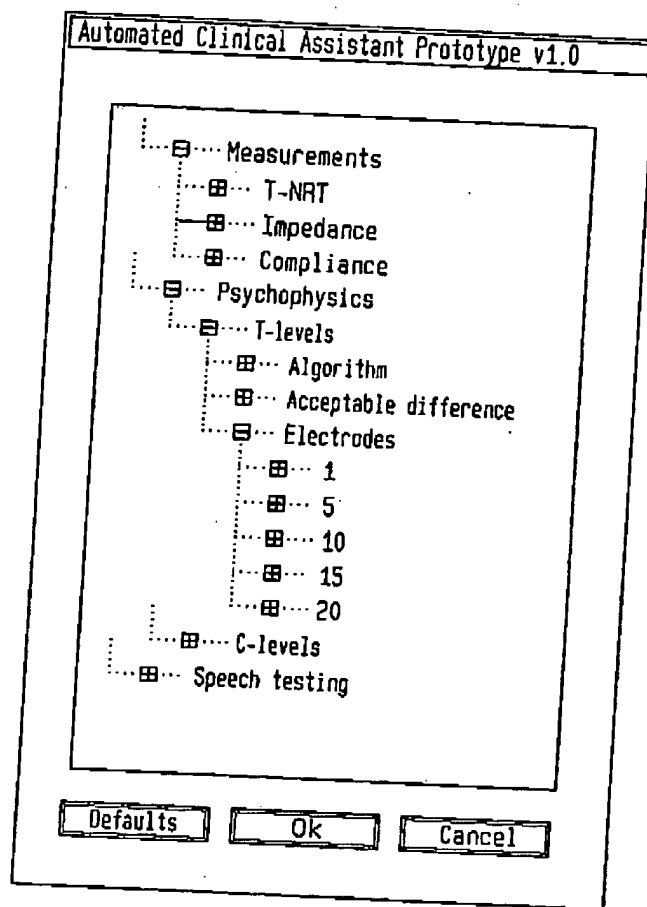

REPLACEMENT SHEET

7/16

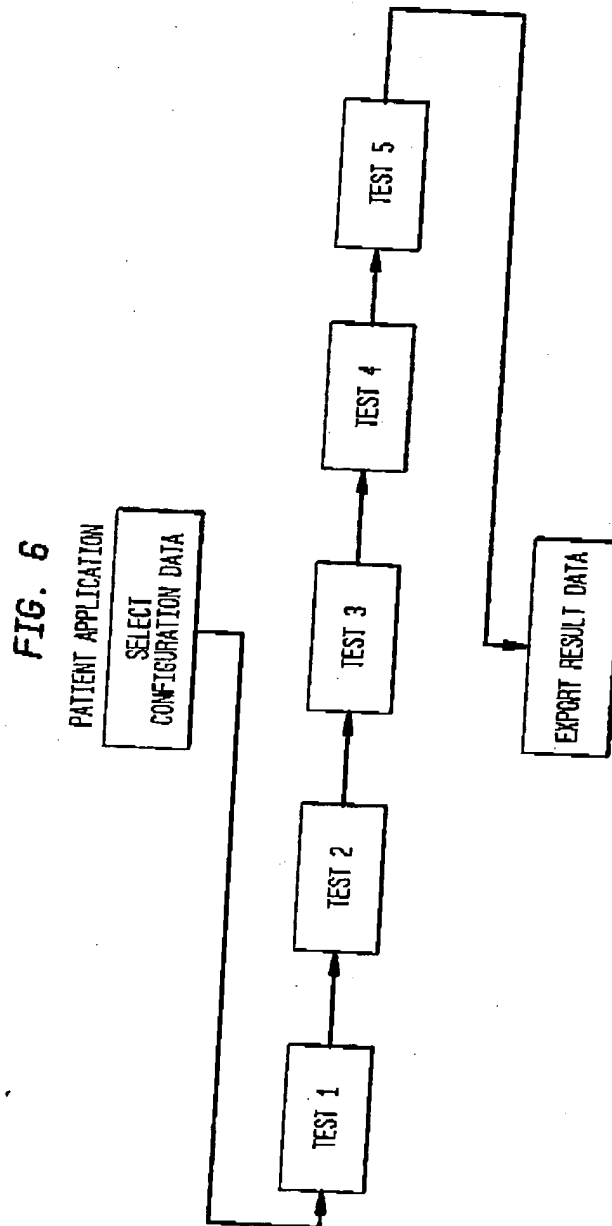

8/16

FIG. 7


Welcome, Bob Peeters.	
<p>We will lead you through different tests.</p> <p>Ask the audiologist for help if something is unclear.</p> <p>Press the NEXT button on the right bottom corner to continue.</p>	

NEXT

9/16

REPLACEMENT SHEET


FIG. 8

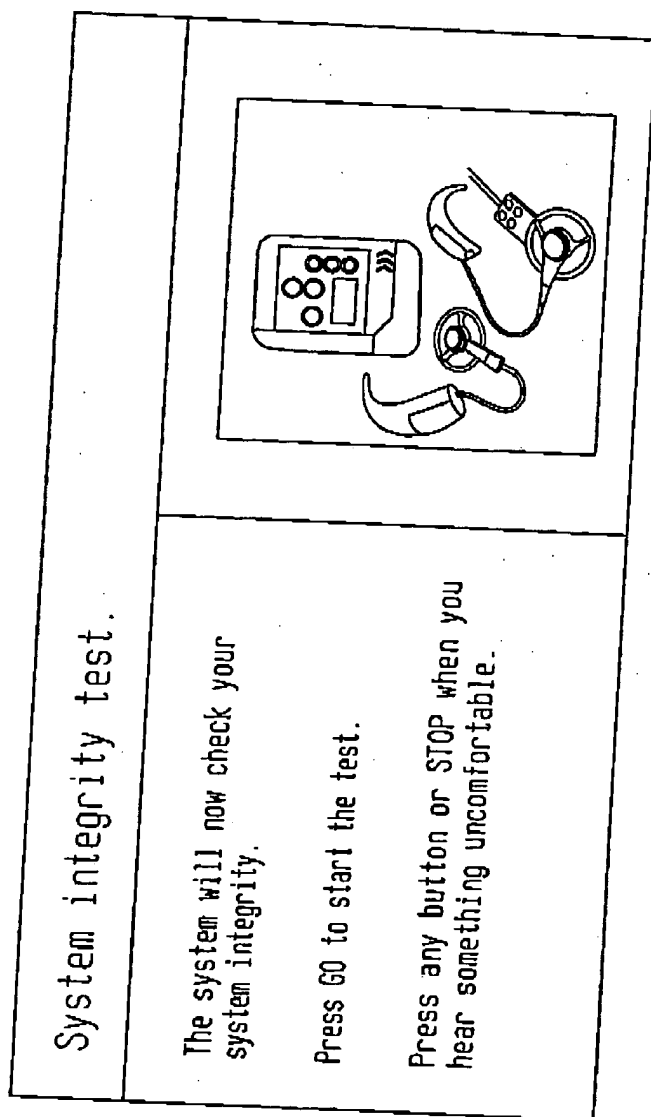

GO


10/16

FIG. 9

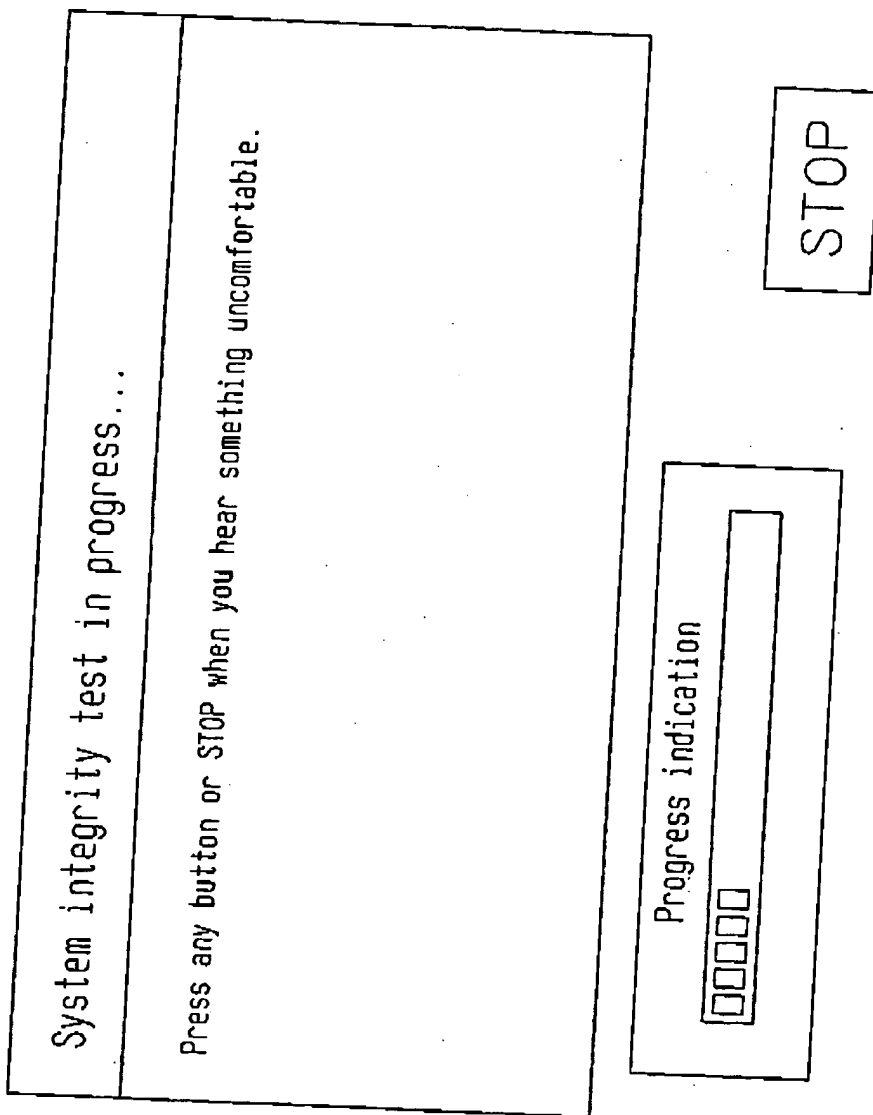

11/16

FIG. 10

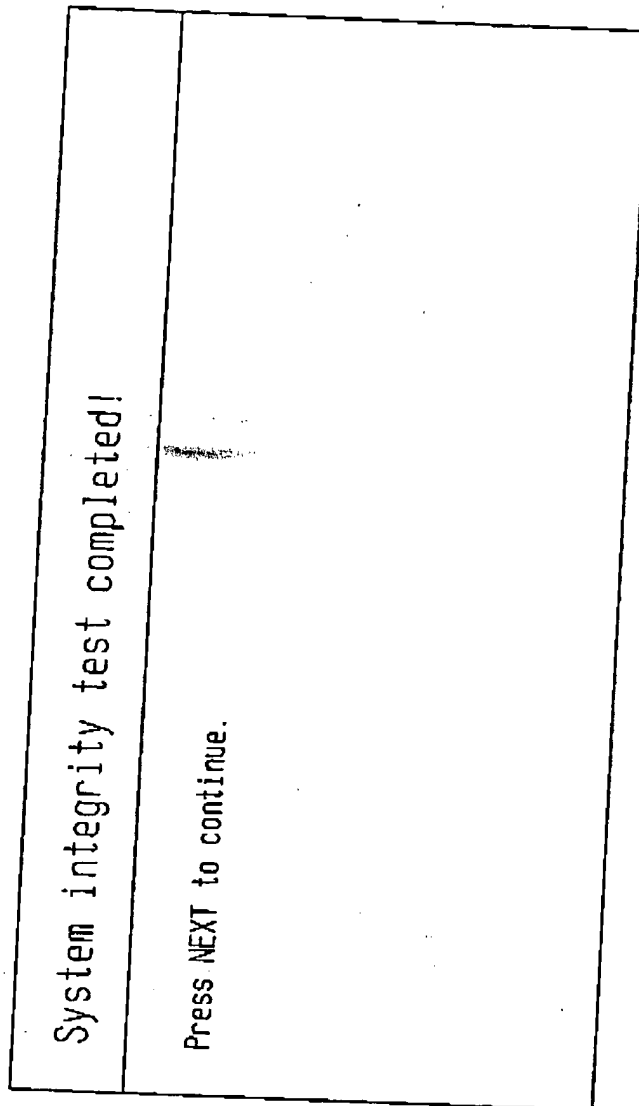


NEXT

12/16

REPLACEMENT SHEET

FIG. 11

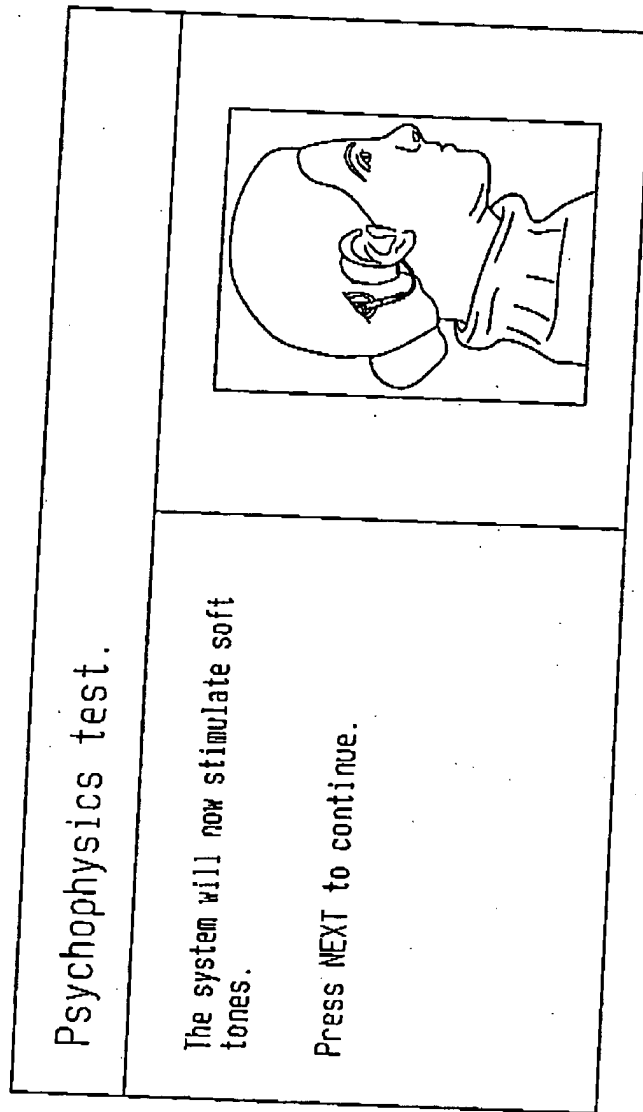

NEXT

13/16

FIG. 12

Psychophysics test in progress...
<p>Press PLAY to start the tone stimulation. Press YES when you hear something. Press NO when you hear nothing. Press any button or STOP when you hear something uncomfortable. You will be unable to hear some tones, since we also test at low levels.</p>

PLAY

YES

NO

STOP

14/16

FIG. 13


Psychophysics test completed!
Press NEXT to continue.

NEXT

REPLACEMENT SHEET

15/16

FIG. 14

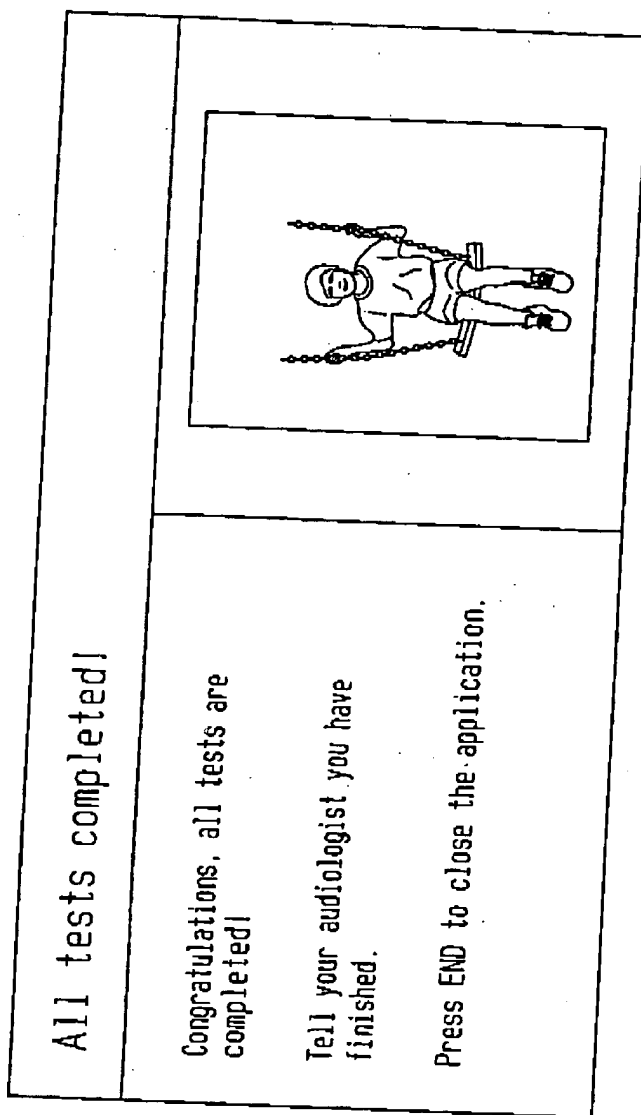

END

REPLACEMENT SHEET

16/16

FIG. 16

